


ICW MD ARM INSTALLATION INSTRUCTIONS

ICWUSA.com, Inc.

If you have any questions, please call 1-800-558-4435


REMOVE COVERS FROM MD ARM

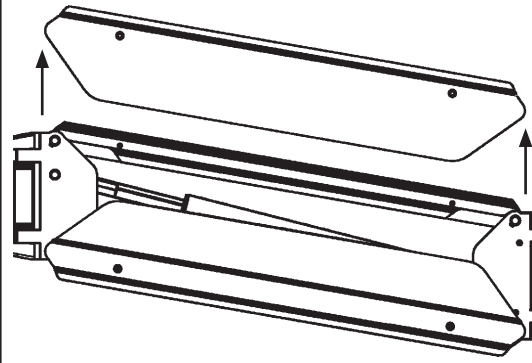

Using a Phillips head screwdriver, remove the four screws from the upper cover, exposing the cable channel.


WARNING - PINCH POINT: Keep fingers away from the inner arm area where the gas spring is located.

The lower cover can also be removed by lowering the arm into the down position, removing the screws and sliding the cover forward off of the arm.

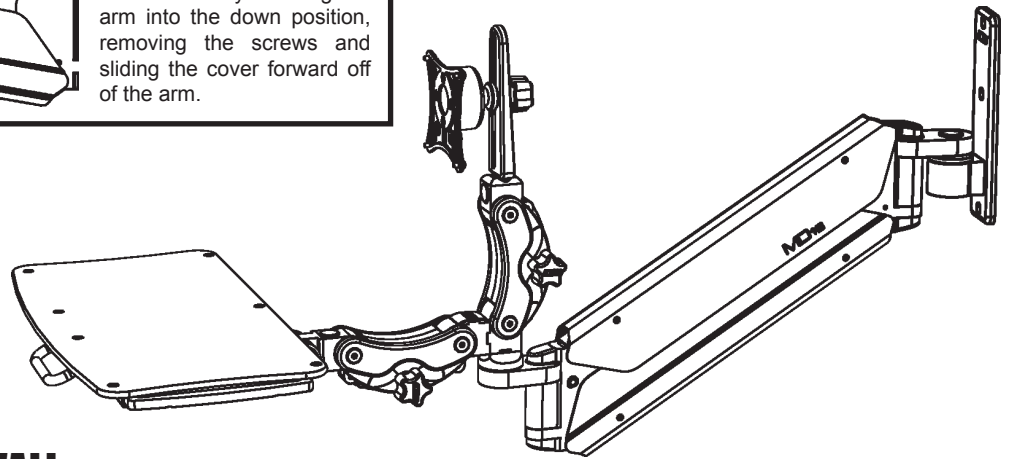

IF MOUNTING DIRECTLY TO WALL

ATTACH MD WALL MOUNT

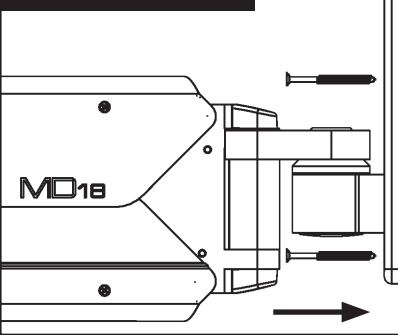


Locate a stud in a wall you intend to mount your arm on. Mark the top hole, drill 11/64 pilot hole and insert an ICW provided #14 screw and tighten slightly. Using a level, mark the 3 lower holes and drill pilot holes, insert the last three #14 screws and with the mount level, tighten all screws securely.

OR

IF MOUNTING TO WALL TRACK

ATTACH WALL PLATE TO TRACK

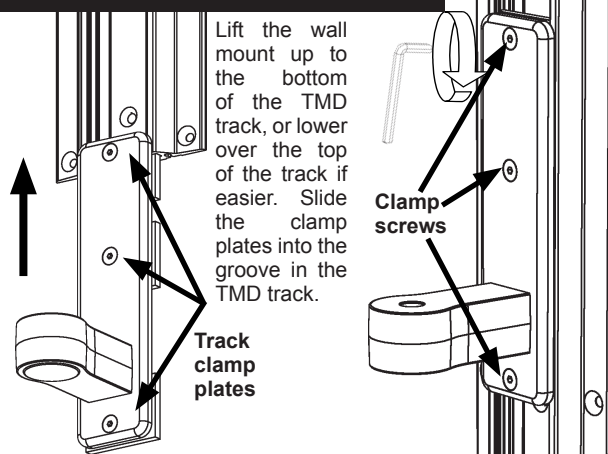


Lift the wall mount up to the bottom of the TMD track, or lower over the top of the track if easier. Slide the clamp plates into the groove in the TMD track.

Once the wall plate is at the height that you want it, use the 5/32 hex key to lock it into place by turning the 3 clamping screws in to place clockwise.

MD ARM INSTALLATION INSTRUCTIONS


ATTACH PARALINK TO MD ARM

Attach the Paralink to MD arm using 3/8 bolt assembly and 1" bearing assembly provided. Insert bolt assembly up through ear at end of arm. Place 1" bearing assembly over bolt on top of ear. Place Paralink over bolt and bearing and turn bolt until Paralink is secure and smoothly turns against the bearing.

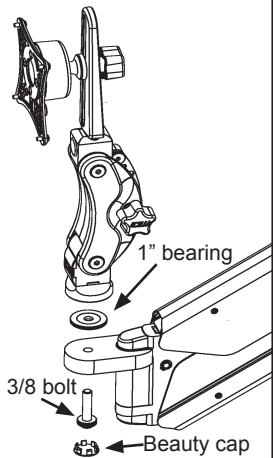


ATTACH VESA TO MONITOR

Attach VESA to monitor using four 4mm screws in the hardware bag.

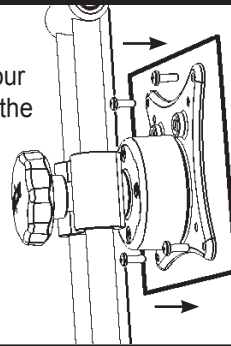

ADJUST PARALINK TILT


Adjust monitor to desired position with ball VESA. Tilt your monitor 50° in any direction. Adjust your monitor between portrait and landscape by rotating ball VESA. Adjust monitor depth by moving the paralink forward or back then tightening the depth adjustment knob.

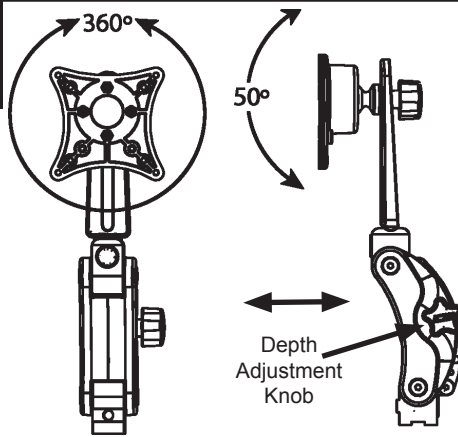

ADJUST BALL VESA TENSION & HEIGHT



Use the slider knob to loosen the slider to adjust the height of the monitor on the Paralink.

Adjust the pivot tension of the ball by gently and evenly tightening or loosening the four screws on the back of the ball VESA.

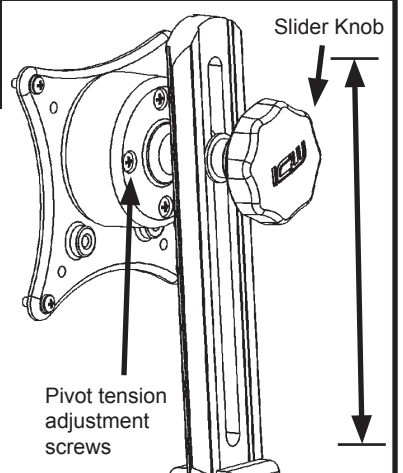

ATTACH THE THBV HANDLE

The THBV is attached to the Paralink and Quicklink by two screws on the back of the VESA plate.

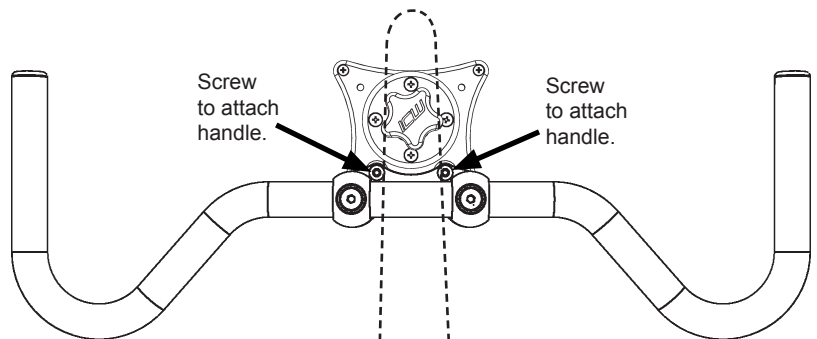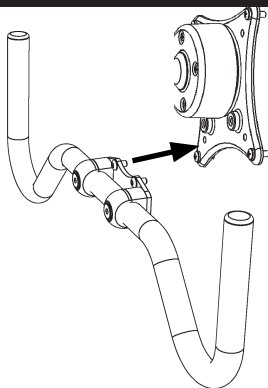


MD ARM INSTALLATION INSTRUCTIONS

IF USING ULTRA KEYBOARD TRAY

ATTACH FLIP UP

1. Remove screws from drop extension using 5/32" hex key.
2. Align holes in keyboard tray with screw holes in drop extension.
3. Attach keyboard tray using the provided screws.

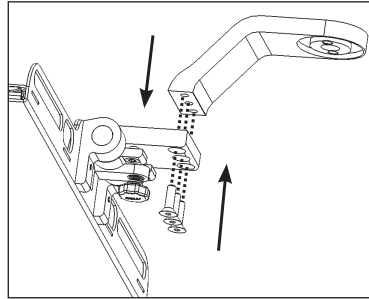


OR

IF USING PARALINK KEYBOARD TRAY


ATTACH PARALINK KEYBOARD TO MONITOR

Attach the Paralink Keyboard Mount to the Monitor Mount by using the 3/8-16 screw and lock washer provided.

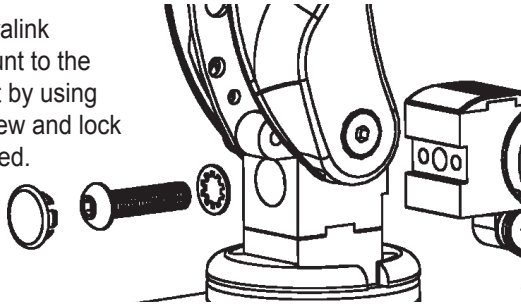


ATTACH QUICK DISCONNECT

1. Remove beauty cap on quick disconnect block.
2. Remove screw using 3/16" hex key.
3. Slide keyboard tray into quick disconnect block.
4. Replace screw and tighten.
5. Replace beauty cap.

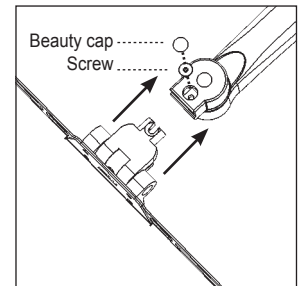

ATTACH COVERS TO MD ARM

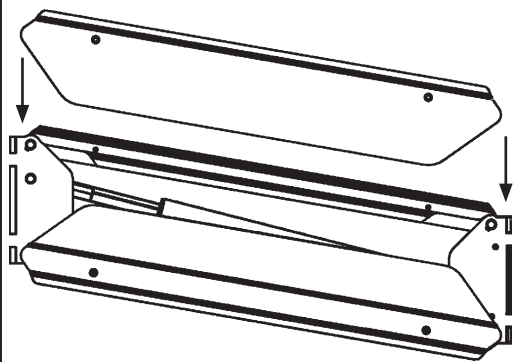


After lowering the arm to the down position, slide on the lower cover. Using a Phillips head screwdriver (NOT POWER TOOLS), reattach the four screws attaching the lower cover.

Attach the top cover by reattaching the four top cover screws using a Phillips head screwdriver (NOT POWER TOOLS).

WARNING - PINCH POINT:
Keep fingers away from the inner arm area where the gas spring is located.

ADJUST MD ARM RESISTANCE

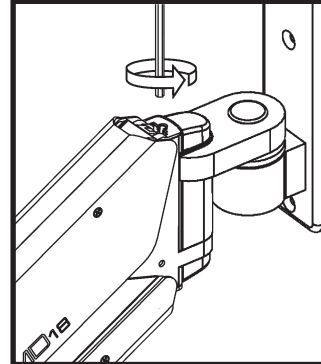

Using the 3/16" t-handle hex wrench provided, turn the screw in the MD arm clockwise to lighten the arm's load resistance, or counter-clockwise to increase the load resistance.